

CBCT-161

DENTAL CBCT


CBCT-161 is used for constancy testing in accordance with the DIN 6868-161 standard.

CBCT-161 includes:

- PMMA cylinder with;160 mm diameter, 40 mm length
- Spirit level and pigment-filled centre markings for easy and reproducible positioning.
- Tripod for universal positioning
- Soft tissue equivalent; PMMA - density $1.20 \pm 0.01 \text{ g/cm}^3$
- Bone equivalent; PVC- density $1.30 - 1.45 \text{ g/cm}^3$
- Air gap

CBCT-161 permits measurement of the following image quality parameters:

- Pixel Intensity Value Linearity
- Noise
- CNR
- Homogeneity
- Artefacts
- MTF

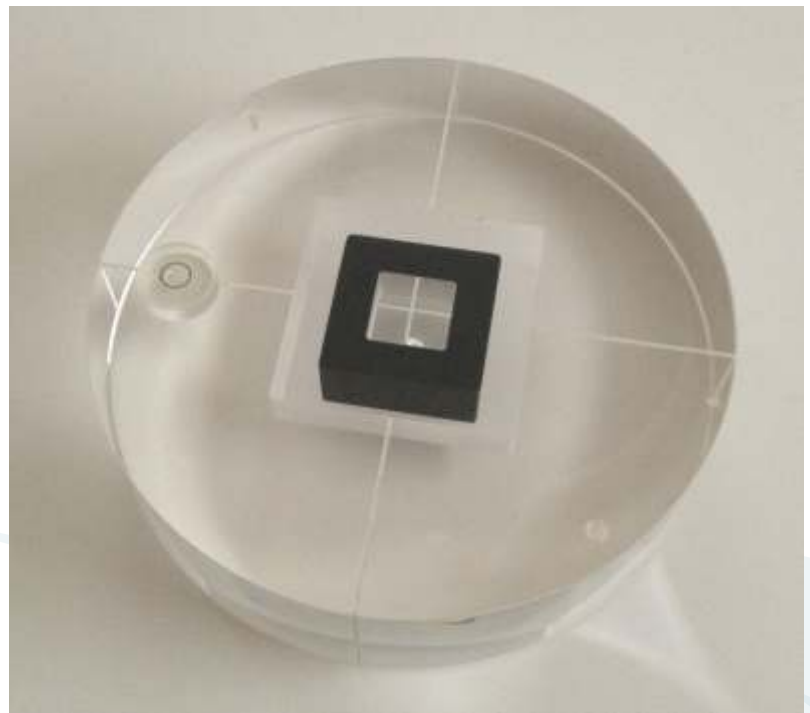

CBCT-161

For more information or to find your regional distributor please visit our website